



FIG. 2

206210-52295001


FIG. 3

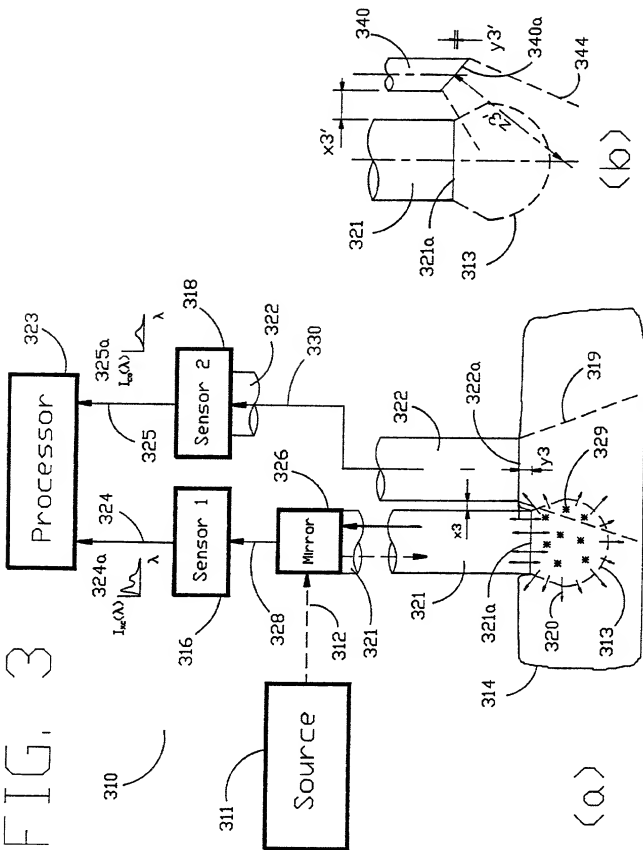


200210" SECESS001

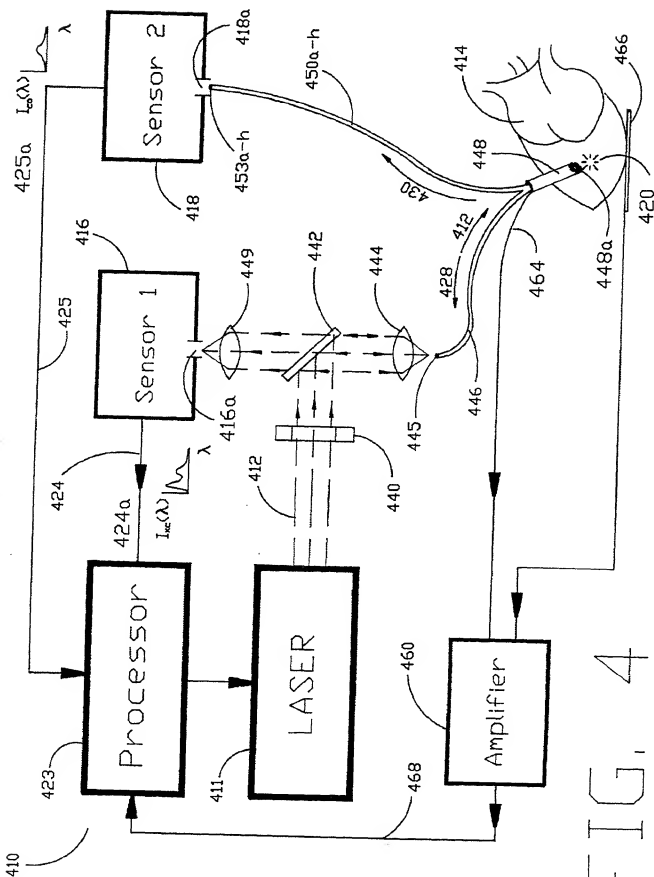

206270-SEE9500F

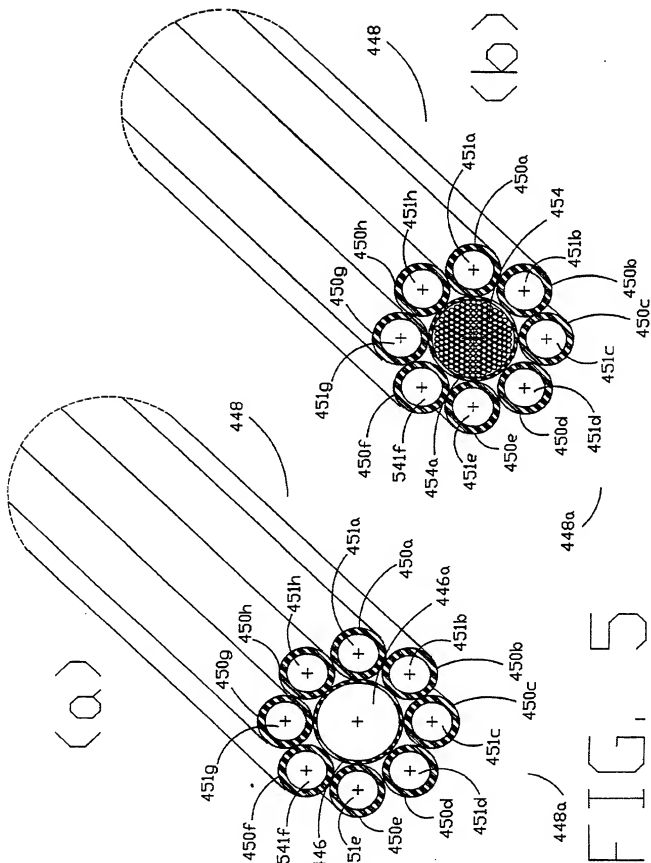

9511

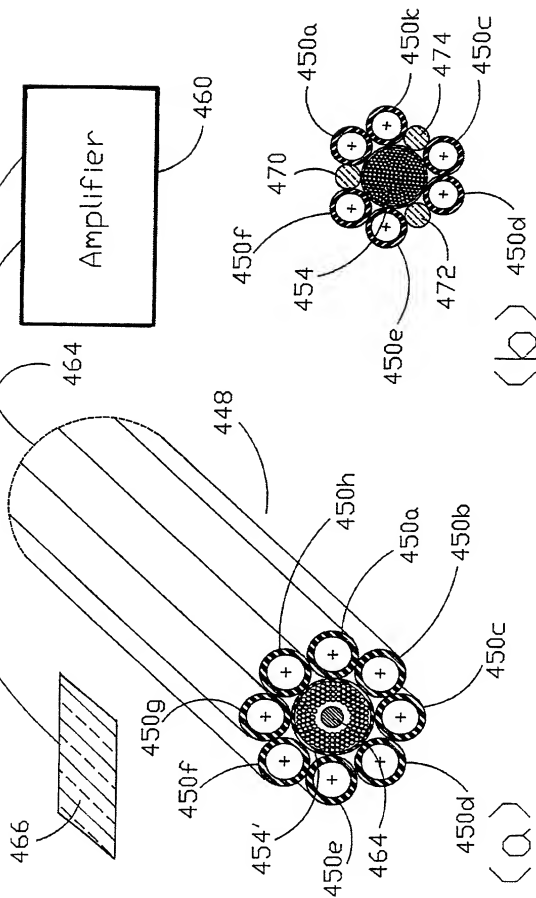

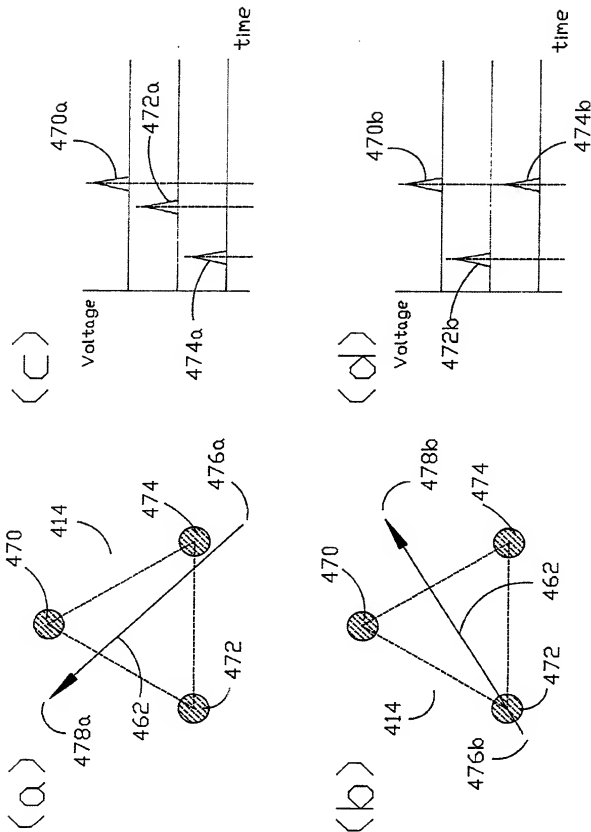



FIG. 7


202210-SEE95001

206210-SEE95001

To /from the
 optical system

FIG. 8

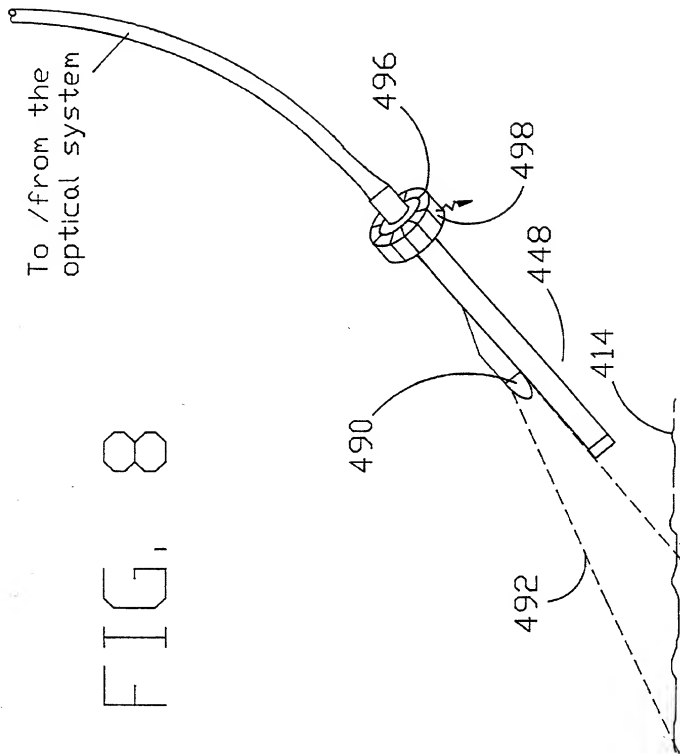

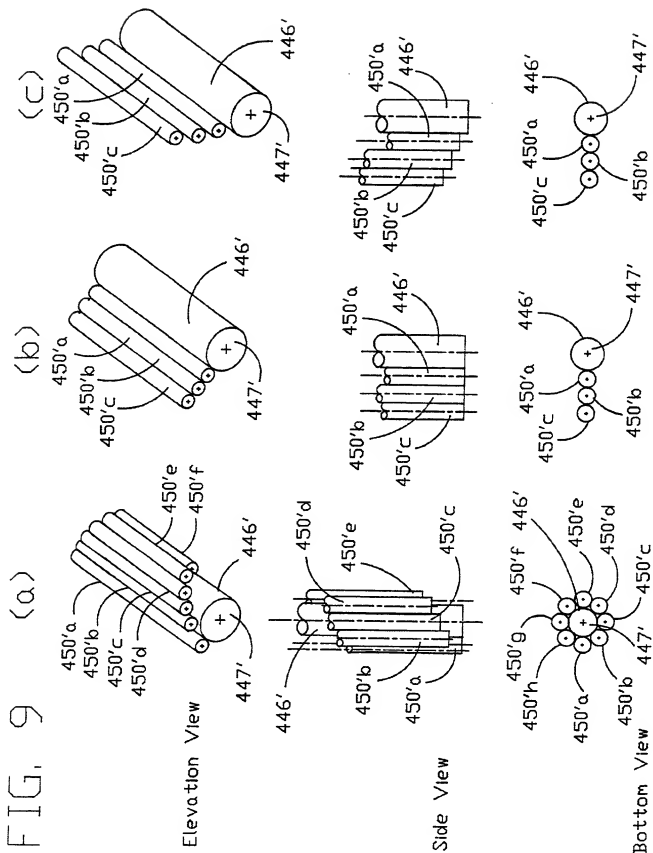

200210-55095001

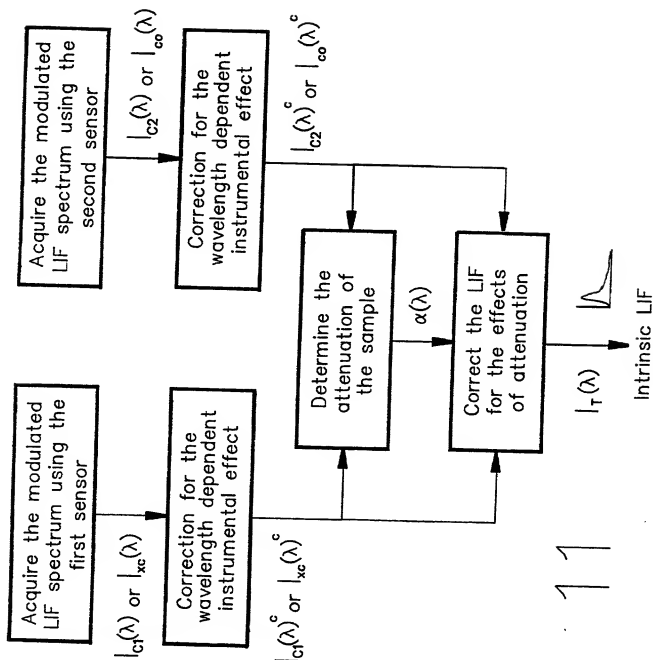


FIG. 11

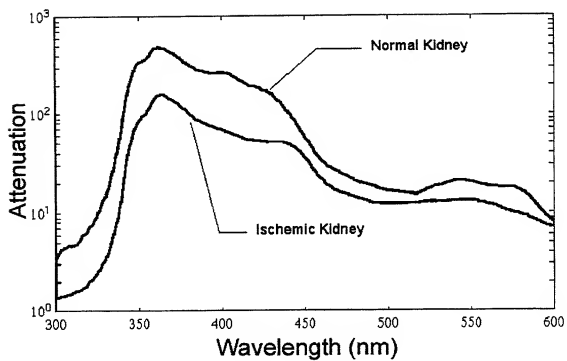


FIG. 12

NEW

Kidney: x = 100, o = 20, + = 0 % O₂ at 5 min.

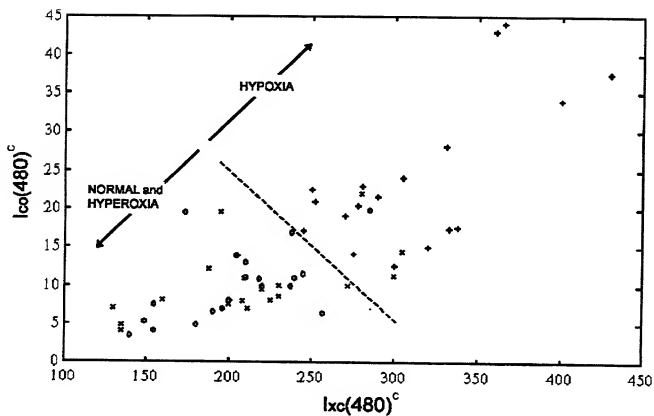


FIG. 13

NEW



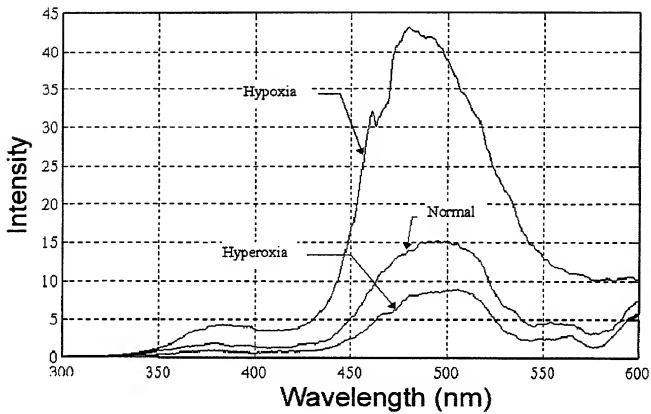


FIG. 14

NEW

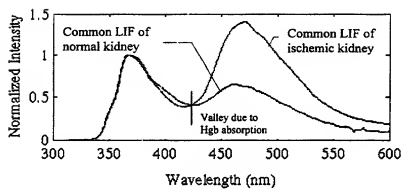


(a)

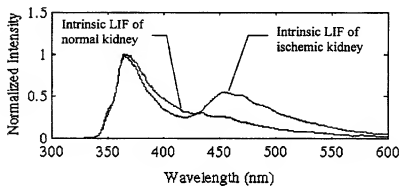


(b)

FIG. 15

NEW

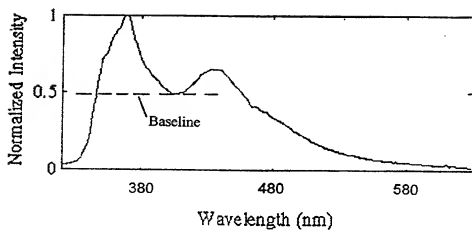


(a)

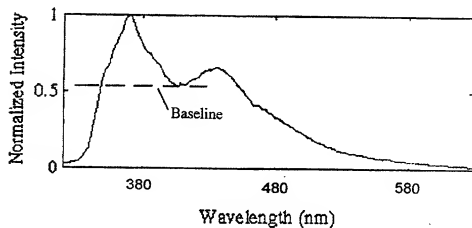


(b)

FIG. 16


NEW

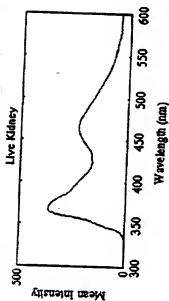


(a)

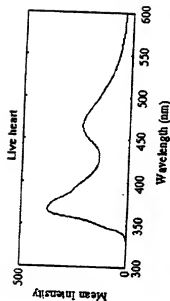

(५)



(c)

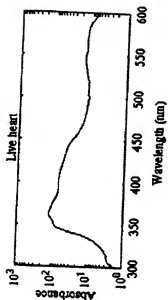

(v)

FIG. 17